


# TurboVap Concentration

## TurboVap Options After Dionex ASE™ Extraction

CONCENTRATION OPTIONS

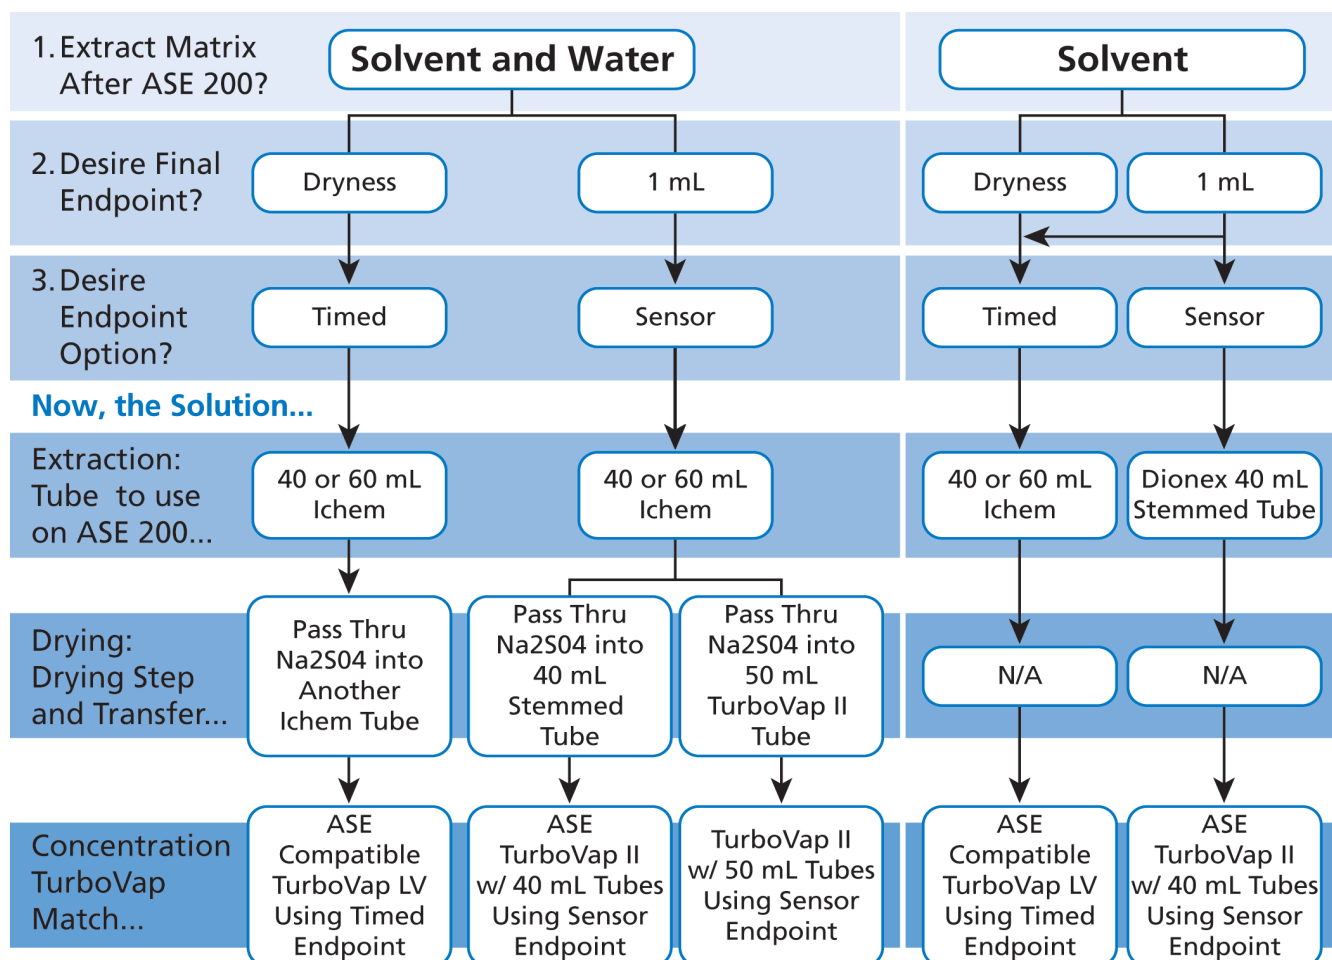

With many labs adapting the new methodology using the Dionex ASE 200 system, Biotage has recognized the need to assist laboratories with their concentration options.

In order to decide which model TurboVap will best fit a laboratory's application, the following questions should be asked, along with following the flowchart on the reverse side:

- After extraction on the Dionex ASE, what is the matrix of my extract?
- After extraction on the Dionex ASE, will the extract require further cleanups or drying steps?
- What other types of samples may require concentration that are not extracted on the ASE, so that I may select the model TurboVap that will be suitable for all types?
- Do I have enough Dionex ASE extracts and enough non-ASE extracts to justify two separate model TurboVaps?
- Does it make sense for me to purchase a standard TurboVap model now, and convert with the ASE compatible kit later?

